


SN# 000577 Lamp Specific Acceptance Test



Model: UV-4000, Profusion	Result	Steady State	Acceptable	Units
Peak Output Wavelength	Pass	369 ✓	365 ± 5	nm
Full Width Half Maximum (FWHM)	Pass	11 ✓	≤ 15	nm
Full Width at 10% Maximum	Pass	23 ✓	≤ 30	nm
Longest Wavelength at Half Maximum	Pass	375 ✓	≤ 377	nm
Max Excitation Irradiance (347-382 nm)	Pass	3607 ✓	≥ 2000	μW/cm ²

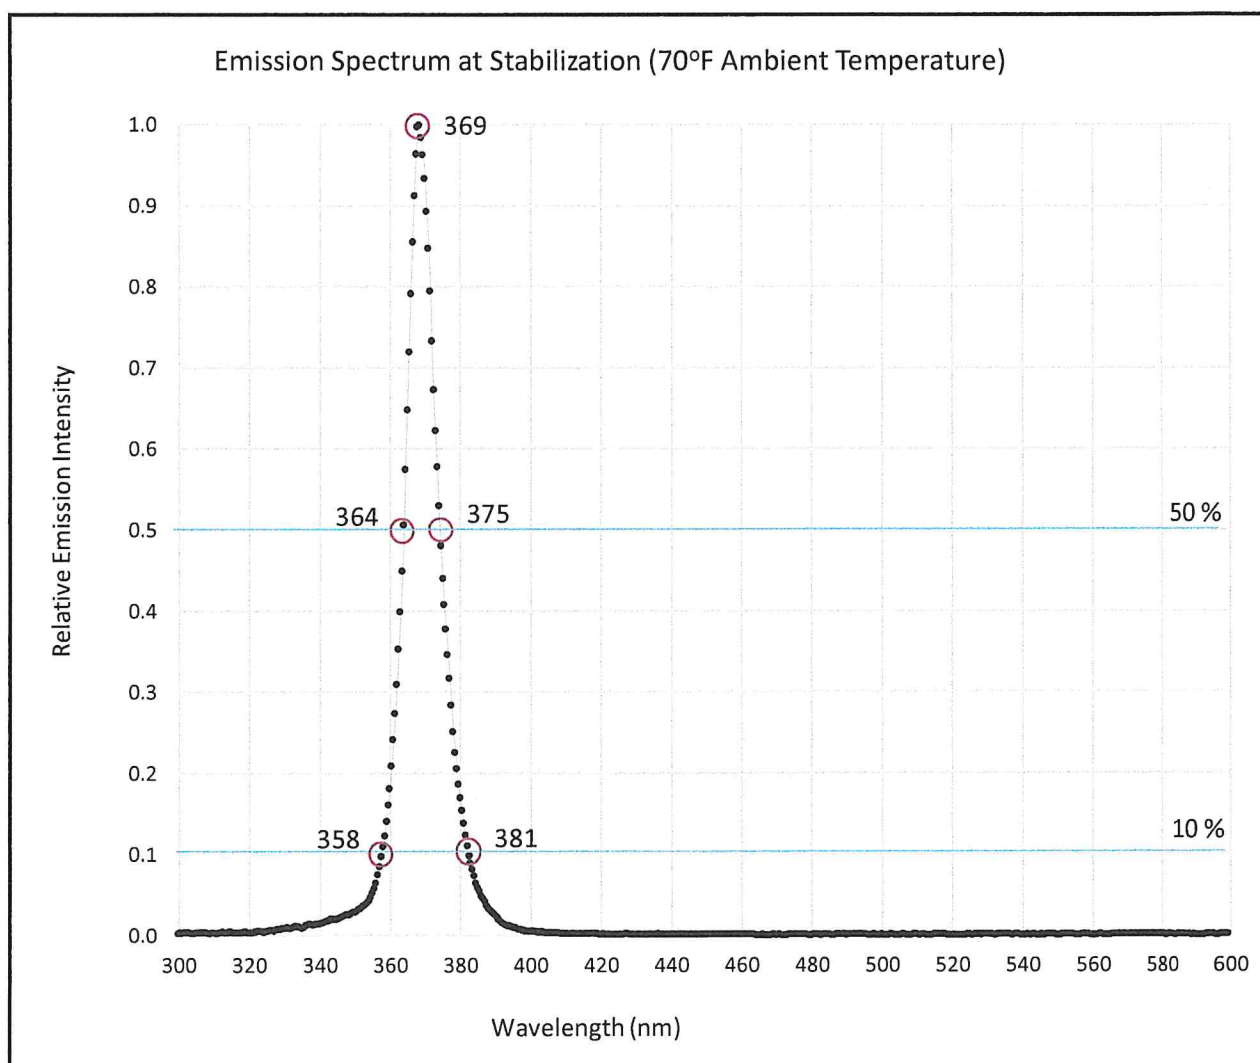

Inspector: MHP
 Date of Certification: 10-23-2025

This lamp has been tested to conform to all requirements of:
 ASTM E3022 ✓ AITM6-1001 ✓ ISO 3059 ✓ RRES 90061 ✓

Emission Spectrum Measured at Stabilization Temperature with Blue-wave UV-25 S/N 22011404, Certificate Number 22011404-UV-CR2-1124



Profusion Series, Certificate of Conformance



SN# 000577	Switch On	Steady State	Elevated Temp*	Acceptable	Units
Peak Output Wavelength	368	369	369	365 ± 5	nm
Full Width Half Maximum (FWHM)	11	11	13	≤ 15	nm
Full Width at 10% Maximum	23	23	26	≤ 30	nm
Longest Wavelength at Half Maximum	374	375	376	≤ 377	nm
Visible Emission at 15 in	9	8	8	≤ 20	Lux
Visible Emission at 36 in	3	3	3	≤ 5	Lux
Irradiated Area at 15 in (>1000 μW/cm ²)	10	9	8	≥ 5	Inch Diameter
Max Excitation Irradiance (347-382 nm)	4,220	3,607	2,600	≥ 2,000	μW/cm ²
Irradiance at Peak Output Wavelength	342	293	210	-	μW/cm ²
Min Working Distance** (< 5000 μW/cm ²)	15	13	12	-	Inches
Max Working Distance** (> 1200 μW/cm ²)	27	25	21	-	Inches
Body Stabilization Temp (70°F Ambient)	-	104	-	≤ 120	°F
Current Ripple	9	9	9	≤ 35	mA peak-peak

* Tested in a 115°F Environment, the maximum ambient temperature where still light meets all requirements

** Profusion series lights use a single LED emitter, thus beam uniformity does not change with working distance (RRES 90061)

